


SERIES 1300 Oxygen Deficiency Monitor¹

Example Installation Configuration¹

For a System with Two Remote Oxygen Sensors
With Optional Horn and Strobes

*Note: For Lighter Gases Such as He,
Consideration Should be Given for Installing
the Remote Sensor at a Higher Elevation.*

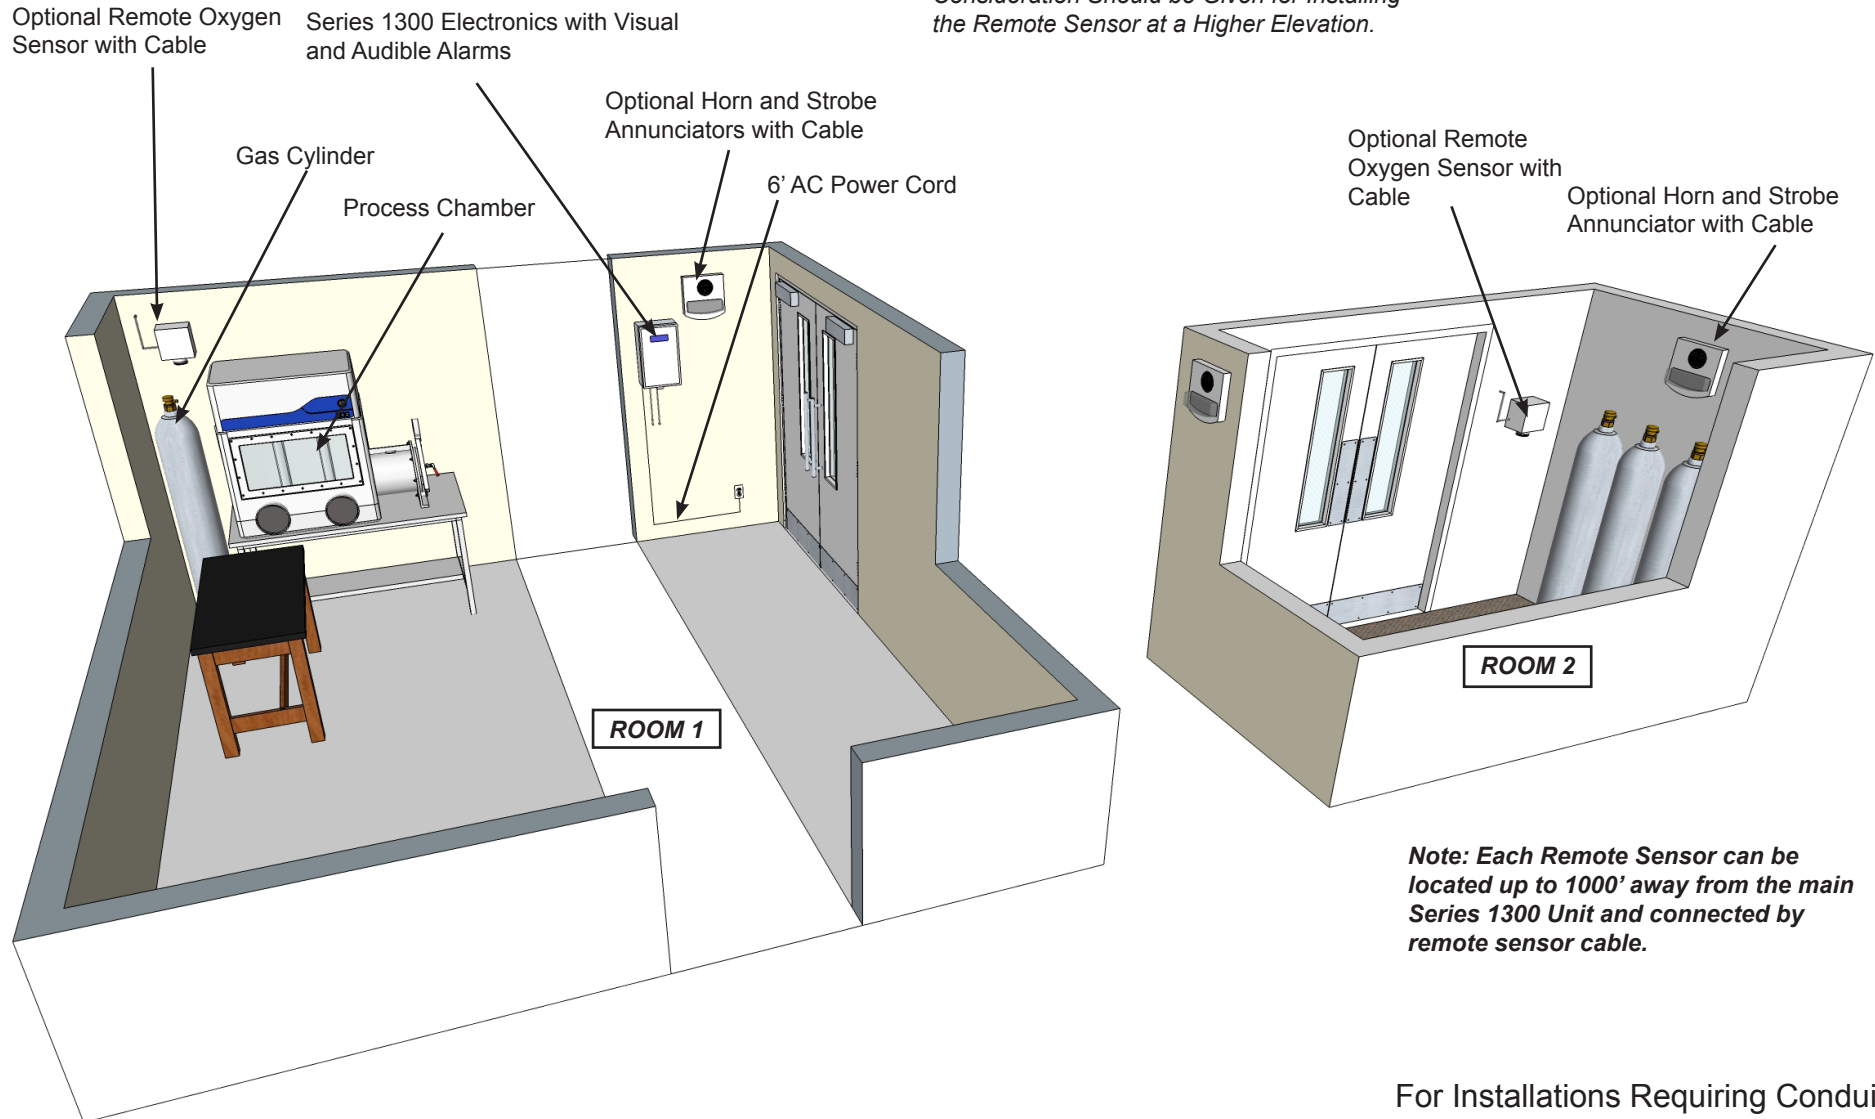

Note: Each Remote Sensor can be located up to 1000' away from the main Series 1300 Unit and connected by remote sensor cable.

For Installations Requiring Conduit,
Please Contact Factory

Note: Horn and Strobe Can be Installed at a Different Location than the Remote Sensor

¹ Disclaimer: The above installation is for example purposes only. It does not represent a specific recommendation by Alpha Omega Instruments. The exact placement of the monitor(s) and sensor(s), as well as the number required, is to be determined by the end user based on the physical layout of the proposed installation.