


SERIES 1300 Oxygen Deficiency Monitor¹

Example Installation Configuration

Oxygen Monitor with Dual Optional Horn and Strobes at Two Entrances

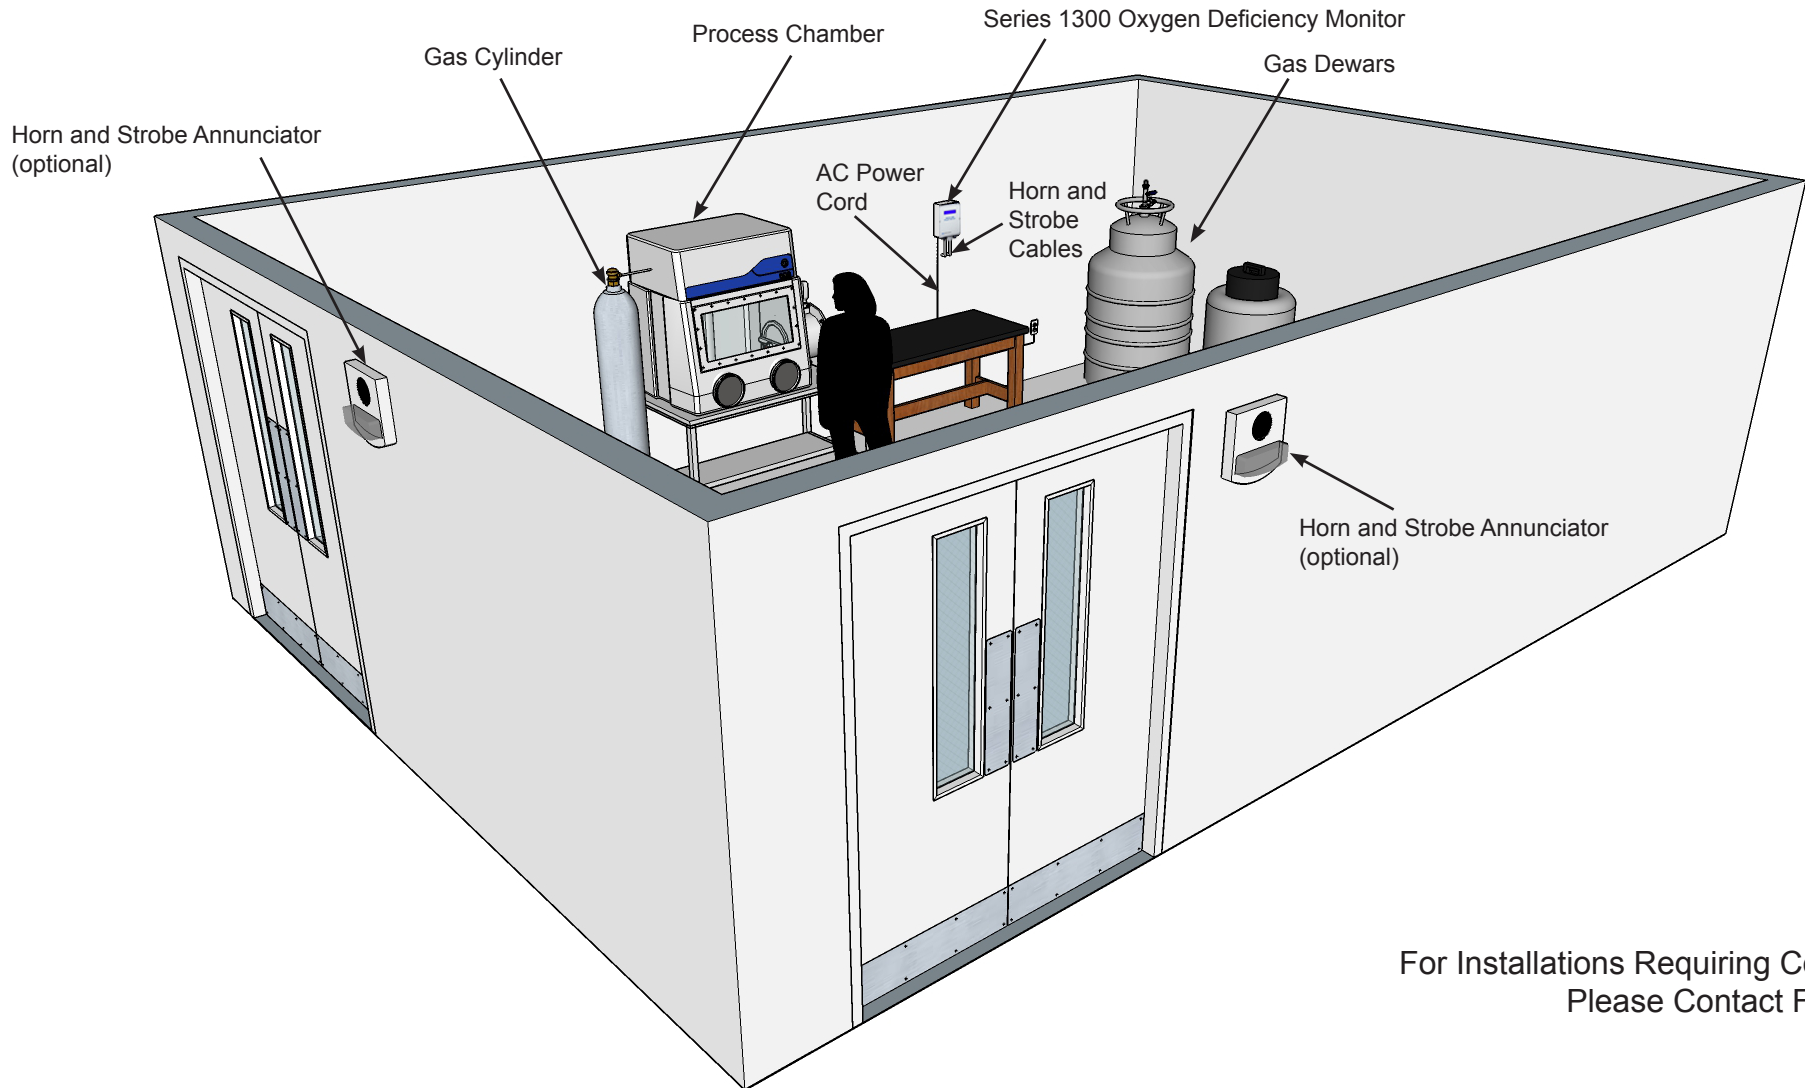

For Installations Requiring Conduit,
Please Contact Factory

¹ Disclaimer: The above installation is for example purposes only. It does not represent a specific recommendation by Alpha Omega Instruments. The exact placement of the monitor(s) and sensor(s), as well as the number required, is to be determined by the end user based on the physical layout of the proposed installation.